

Technical Manual

ChromaDazzle Glycolysis Assay Kit

Catalogue Code: BA0086

Pack Size: 100 assays

Research Use Only

DESCRIPTION

GLYCOLYSIS is one of the major metabolic pathways cells undergo to produce energy and results in the production of pyruvate. One of the eventual fates of pyruvate from this process is lactate dehydrogenase converting it to L-lactate via lactic acid fermentation allowing L-lactate to serve as an indicator of glycolysis.

The Assay Genie ChromaDazzle Glycolysis Assay Kit is based on measuring the production of L-Lactate from glycolysis in cells. L-Lactate that is secreted into the cell media is quantified using a coupled reaction involving the lactate dehydrogenase catalyzed oxidation of L-lactate that generates pyruvate and NADH which reduces a formazan dye. The intensity of the reduced dye, measured at 565 nm, is directly proportional to the L-lactate concentration in the sample, which in turn is directly proportional to the glycolytic rate of the cells.

KEY FEATURES

Fast and sensitive. Use of 5 μL sample. Linear detection range up to 10 mM L-lactate in 96-well plate assay.

Convenient. The procedure involves adding a single working reagent, and reading the absorbance after 30 minutes. Room temperature assay. No 37°C heater is needed.

High-throughput. "Add-mix-read" type assay. Can be readily automated as a high-throughput 96-well plate assay for thousands of samples per day.

APPLICATIONS

Direct Assays: L-Lactate produced by glycolysis in cell samples. Screening of glycolysis inhibitors and effect of drugs on glycolysis.

KIT CONTENTS (100 TESTS IN 96-WELL PLATES)

Reagent: 12 mL

Standard: 250 μL

Storage conditions. The kit is shipped on ice. Store all components at -20°C upon receiving. Shelf life: 6 months after receipt.

Precautions: reagents are for research use only. Briefly centrifuge tubes before opening. Equilibrate all components to room temperature prior assay. Normal precautions for laboratory reagents should be exercised while using the reagents. Please refer to Material Safety Data Sheet for detailed information.

PROCEDURES

Sample Preparation: Plate cells in media of choice. After allowed enough time for cells to adhere to plate, remove media and replace with low percentage FBS media (FBS \leq 1% or serum free media). For suspension cells, seed at desired cell number in low percentage FBS media. Set 2 mL of media aside for making standards. Add any treatments or compounds being tested at this step as well. Allow cells to propagate to desired confluence. Remove media for assay.

Procedure using 96-well plate

1. **Standards.** Prepare 1 mL of 10 mM Premix by mixing 10 μL of the Standard (0.5 M) and 490 μL of the low percentage FBS media used for the cells. Dilute standards in 1.5-mL centrifuge tubes as described in the Table.

No	Premix + Media	L-Lactate (mM)
1	100 μL + 0 μL	10
2	60 μL + 40 μL	6
3	30 μL + 70 μL	3
4	0 μL + 100 μL	0

2. Transfer 5 μL standards into separate wells of a clear, flat-bottom 96-well plate. Transfer 5 μL of each sample into separate wells. (For improved accuracy, we recommend running all wells in at least duplicate)

3. Add 95 μL Reagent to the *four Standards* and the *Sample Wells*. Tap plate to mix briefly and thoroughly. Incubate 30 minutes at room temperature.
4. Read optical density at 565 nm (520-600 nm).

CALCULATION

Subtract the blank value (#4) from the standard values and plot the ΔOD against standard concentrations. Determine the slope and calculate the formate concentration of Sample as follows:

$$[\text{L-Lactate}] = \frac{\text{OD}_{\text{SAMPLE}} - \text{OD}_{\text{BLANK}}}{\text{Slope (mM}^{-1})} \quad (\text{mM})$$


$\text{OD}_{\text{SAMPLE}}$ and OD_{BLANK} are optical density readings of the Sample and Media Blank (#4), respectively.

Conversions: 1 mM L-lactate equals 9.01 mg/dL, or 90.1 ppm.

Note: This assay reaches OD values greater than 1.0. If your plate reader is not accurate to values that high, you may choose to construct a modified 0, 1.5, 3, 5 mM standard curve instead.


MATERIALS REQUIRED, BUT NOT PROVIDED

Pipetting devices, centrifuge tubes, clear flat-bottom 96-well plates (e.g. VWR cat# 82050-760), and plate reader.

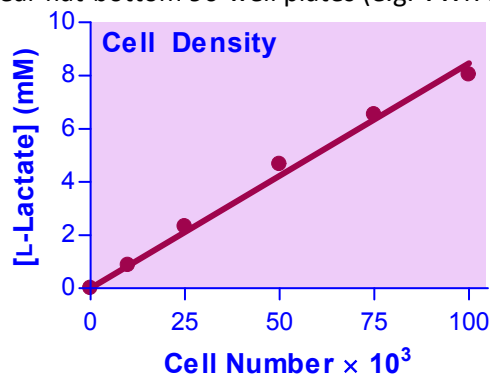

Cell Density and Rate of Glycolysis

HL-60 cells seeded at varying cell densities in RPMI medium



Glycolysis Inhibition

PANC1 cells treated with varying concentrations of 2-deoxy-D-glucose in DMEM medium

LITERATURE

1. TeSlaa, T., et al (2014). Techniques to Monitor Glycolysis. *Methods Enzymol* 542: 91-114.
2. Kim, J., et al (2006). Cancer's Molecular Sweet Tooth and the Warburg Effect. *Cancer Res* 66.18: 8927-8930.
3. Rogatzki, M., et al (2015). Lactate is Always the End Product of Glycolysis. *Front Neurosci* 9: 22.

Contact Details

Dublin, Ireland

Email: info@assaygenie.com

Web: www.assaygenie.com

Technical Support: Techsupport@assaygenie.com