

## **Technical Manual**

### **ColorFluor Glycerol Assay Kit**

**Catalogue Code: BA0115**

**Pack Size: 200 assays**

**Research Use Only**

## DESCRIPTION

**GLYCEROL** [*GLYCERIN* or *GLYCERINE*,  $C_3H_5(OH)_3$ ] is widely used in foods, beverages and pharmaceutical formulations. It is also a main by-product of biodiesel production. Simple, direct and automation-ready procedures for measuring glycerol concentrations find wide applications. The Assay Genie ColorFluor Glycerol Assay Kit glycerol assay uses a single Working Reagent that combines glycerol kinase, glycerol phosphate oxidase and color reactions in one step. The color intensity of the reaction product at 570nm or fluorescence intensity at  $\lambda_{em}/\lambda_{ex} = 585/530nm$  is directly proportional to glycerol concentration in the sample.

## KEY FEATURES

**Sensitive and accurate.** Use as little as 10  $\mu L$  samples. Linear detection range in 96-well plate: 10 to 1000  $\mu M$  (92  $\mu g/dL$  to 9.2 mg/dL) glycerol for colorimetric assays and 2 to 50  $\mu M$  for fluorimetric assays.

**Simple and convenient.** The procedure involves addition of a single working reagent and incubation for 20 min at room temperature, compatible for HTS assays.

**Improved reagent stability.** The optimized formulation has greatly enhanced the reagent and signal stability.

## APPLICATIONS:

**Direct Assays:** glycerol in biological samples (e.g. serum and plasma).

**Drug Discovery/Pharmacology:** effects of drugs on glycerol metabolism.

**Food and Beverages:** glycerol in food, beverages, pharmaceutical formulations etc.

## KIT CONTENTS

**Assay Buffer:** 24 mL    **Enzyme Mix:** 500  $\mu L$     **ATP:** 250  $\mu L$

**Dye Reagent:** 220  $\mu L$     **Standard:** 100  $\mu L$  100 mM Glycerol

**Storage conditions.** The kit is shipped on ice. Store all components at  $-20^{\circ}C$ . Shelf life of 12 months after receipt.

**Precautions:** reagents are for research use only. Normal precautions for laboratory reagents should be exercised while using the reagents. Please refer to Material Safety Data Sheet for detailed information.

## COLORIMETRIC 96-WELL PROCEDURE

*Note:* SH-group containing reagents (e.g. mercaptoethanol, DTT) may interfere with this assay and should be avoided in sample preparation.

1. Equilibrate all components to room temperature. Keep thawed Enzyme Mix in a refrigerator or on ice. Dilute standard in distilled water as follows (diluted standards can be used for future assays when stored refrigerated).

No	STD + H <sub>2</sub> O	Vol ( $\mu L$ )	Glycerol (mM)
1	10 $\mu L$ + 990 $\mu L$	1000	1.0
2	6 $\mu L$ + 994 $\mu L$	1000	0.6
3	3 $\mu L$ + 997 $\mu L$	1000	0.3
4	0 $\mu L$ + 1000 $\mu L$	1000	0

Transfer 10  $\mu L$  standards and 10  $\mu L$  samples into separate wells of a clear 96-well plate.

2. For each reaction well, mix 100  $\mu L$  Assay Buffer, 2  $\mu L$  Enzyme Mix, 1  $\mu L$  ATP and 1  $\mu L$  Dye Reagent in a clean tube. This Working Reagent should be used on the same day of preparation. Transfer 100  $\mu L$  Working Reagent into each reaction well. Tap plate to mix.

3. Incubate 20 min at room temperature. Read optical density at 570nm (550-585nm).

**Note:** if the Sample OD is higher than the Standard OD at 1.0 mM, dilute sample in water and repeat the assay. Multiply result by the dilution factor.

### CALCULATION

Subtract blank OD (water, #4) from the standard OD values and plot the OD against standard concentrations. Determine the slope using linear regression fitting. The glycerol concentration of Sample is calculated as

$$[\text{Glycerol}] = \frac{\text{OD}_{\text{SAMPLE}} - \text{OD}_{\text{H}_2\text{O}}}{\text{Slope}} \quad (\text{mM})$$

$\text{OD}_{\text{SAMPLE}}$  and  $\text{OD}_{\text{H}_2\text{O}}$  are optical density values of the sample and water. **Conversions:** 1mM glycerol equals 9.2 mg/dL, 92 ppm.

### FLUORIMETRIC 96-WELL PROCEDURE

For fluorimetric assays, the linear detection range is 2 to 50  $\mu\text{M}$  glycerol. Mix 10  $\mu\text{L}$  100 mM Standard with 990  $\mu\text{L}$   $\text{H}_2\text{O}$  (final 1 mM).

No	1 mM STD + $\text{H}_2\text{O}$	Vol ( $\mu\text{L}$ )	Glycerol (mM)
1	50 $\mu\text{L}$ + 950 $\mu\text{L}$	1000	0.050
2	30 $\mu\text{L}$ + 970 $\mu\text{L}$	1000	0.030
3	15 $\mu\text{L}$ + 985 $\mu\text{L}$	1000	0.015
4	0 $\mu\text{L}$ + 1000 $\mu\text{L}$	1000	0

Dilute standards as above. Transfer 10  $\mu\text{L}$  standards and 10  $\mu\text{L}$  samples into separate wells of a *black* 96-well plate.

Add 100  $\mu\text{L}$  Working Reagent (see *Colorimetric Procedure*). Tap plate to mix.


Incubate 20 min at room temperature and read fluorescence at  $\lambda_{\text{ex}} = 530\text{nm}$  and  $\lambda_{\text{em}} = 585\text{nm}$ .

The glycerol concentration of Sample is calculated as

$$[\text{Glycerol}] = \frac{F_{\text{SAMPLE}} - F_{\text{H}_2\text{O}}}{\text{Slope}} \quad (\text{mM})$$

### MATERIALS REQUIRED, BUT NOT PROVIDED

Pipeting devices, centrifuge tubes, Clear flat-bottom 96-well plates, black 96-well plates (e.g. Corning Costar) and plate reader.

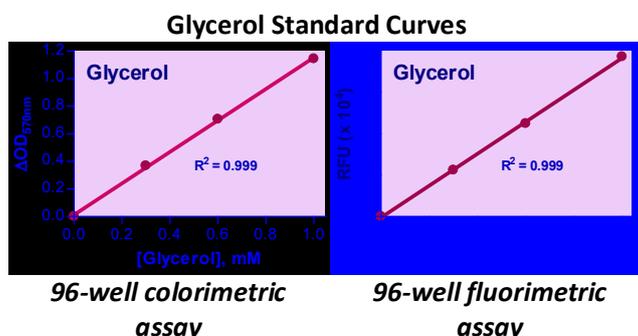

**PUBLICATIONS**

1. Bahar, B et al. A potential role of IL-6 in the chitooligosac-charide-mediated inhibition of adipogenesis (2011). Br J Nutr. 106(8):1142-1153.
2. Drew, BG et al (2011). Reconstituted high-density lipoprotein infusion modulates fatty acid metabolism in patients with type 2 diabetes mellitus. J Lipid Res 52(3):572-581.
3. Wachtler, B et al (2011). From attachment to damage: defined genes of Candida albicans mediate adhesion, invasion and damage during interaction with oral epithelial cells. PLoS One 6(2):e17046.

**Contact Details**

**Dublin, Ireland**

**Email:** [info@assaygenie.com](mailto:info@assaygenie.com)

**Web:** [www.assaygenie.com](http://www.assaygenie.com)

**Technical Support:** [Techsupport@assaygenie.com](mailto:Techsupport@assaygenie.com)

Copyright © 2017 ReagentBio, All Rights Reserved. All information / detail is correct at time of going to print.