

Technical Manual

Dual Luciferase Reporter Assay Kit

Catalogue Code: BA0180


Pack Size: 100 assays

Research Use Only

DESCRIPTION

The accuracy of reporter assays can be improved by utilizing a dual reporter system. One of the reporter genes is correlated with the promoter of interest and is used to assess the effects of specific experimental conditions, while the second reporter is used as a control and serves as a baseline response. The SuperLight™ Dual-Luciferase Reporter Gene Assay allows for the sequential measurement of the activity of two different luciferases, firefly (FFL) and Renilla (RL), in a single sample. The firefly luciferase luminescence is measured first by addition of the FFL Reagent. Next, the RL Reagent is added to the same well. The RL Reagent simultaneously quenches the firefly luciferase luminescence and initiates the Renilla luciferase reaction. The light production of both reactions can be conveniently measured on a luminometer.

Reaction schemes:



This bioluminescent dual reporter gene assay is extremely sensitive and is especially suitable for quantifying dual luciferase expression in recombinant cells or in cell free transcription/translation reactions. Assays can be performed in tubes, cuvettes or multi-well plates.

KEY FEATURES

High sensitivity and wide detection range: detection of as little of 2 fg luciferase.

Compatible with routine laboratory and HTS formats: assays can be performed in tubes or microplates, and measured with any luminometer.

Can be readily automated on HTS liquid handling systems.

Fast and convenient: three step assay allows detection of dual luciferase levels within 20 minutes.

APPLICATIONS

Gene Regulation: gene expression level, characterization of promoter activity, modulation of gene expression by receptors, transcription factors and small molecules.

Drug Discovery: high-throughput screen for gene modulators.

KIT CONTENTS (100 ASSAYS IN 96-WELL PLATES)

Lysis Buffer: 25 mL **FFL Reagent:** 25 mg

Assay Buffer: 25 mL **RL Reagent:** 400 mg

Storage conditions: The kit is shipped at room temperature. Store all reagents at -20 °C.

Shelf life: 12 month after receipt.

Precautions: reagents are for research use only. Normal precautions for laboratory reagents should be exercised while using the reagents. Please refer to Material Safety Data Sheet for detailed information.

ASSAY PROCEDURES

Reagent Preparation: fresh reconstitution of the FFL and RL Reagents in Assay Buffer is recommended. Calculate the amount of each reagent needed (100 μ L of each per assay for 96 well plates or 25 μ L per assay for 384 well plates) and weigh out sufficient amounts of each reagent (2 mg/mL for FFL Reagent and 35 mg/mL for RL Reagent). Gently shake each reconstituted reagent until they are completely dissolved (~10 min). The reconstituted FFL Reagent is stable for up to 4 weeks when stored at -20 $^{\circ}$ C; however, prolonged storage of reconstituted RL Reagent is not recommended and ideally it should be used within 4 hours.

Sample Preparation

1. Remove media from cell cultures and wash cells with PBS.
2. Add enough Lysis Buffer to fully cover the cell monolayer (e.g. 50 μ L per well of a 96 well plate) and place culture plates on an orbital shaker. Gently shake at RT for 15 min.
3. Transfer lysates to tubes for storage (lysates can be stored for 8 hours on ice or overnight at -20 $^{\circ}$ C). Alternatively, the dual luciferase assay can be performed directly in the culture plate if cells were cultured in opaque plates.

Dual Luciferase Assay Procedure

1. If not assaying directly in the culture plate, transfer lysate to an opaque white plate (50 μ L for 96 well plates, 12.5 μ L for 384 well plates).
2. Add reconstituted FFL Reagent to each well. (100 μ L for 96 well plates, 25 μ L for 384 well plates).
3. Measure the firefly luciferase luminescence on a luminometer. The integration time can be 1 sec to 2 min depending on the luciferase expression level and instrument sensitivity. For most luminometers (Berthold Luminometer, LIL Analyst, Top Count, MicroBeta Counters, CLIPR and LeadSeeker), integration 1 to 5 sec is appropriate.
4. Add reconstituted RL Reagent to each well and gently tap to mix. (100 μ L for 96 well plates, 25 μ L for 384 well plates).
5. Measure Renilla luciferase luminescence on a luminometer.

DATA ANALYSIS

The peroxidase activity in a sample is computed as follows:

$$\text{Peroxidase Activity} = \frac{R_{\text{SAMPLE}} - R_{\text{BLANK}}}{R_{\text{RESORUFIN}} - R_{\text{H}_2\text{O}}} \square \frac{[\text{Resorufin}] (\mu\text{M})}{t (\text{min})} \square \frac{\text{Reaction Vol} (\mu\text{L})}{\text{Sample Vol} (\mu\text{L})} \square n$$

$$= \frac{R_{\text{SAMPLE}} - R_{\text{BLANK}}}{R_{\text{RESORUFIN}} - R_{\text{H}_2\text{O}}} \square [\text{Resorufin}] (\mu\text{M}) \square n \quad (\text{U/L})$$

where R_{SAMPLE} , R_{BLANK} , $R_{\text{RESORUFIN}}$ and $R_{\text{H}_2\text{O}}$ are OD or fluorescence readings of the Sample, Sample Blank, Resorufin and Water respectively. n is the sample dilution factor. The [Resorufin] is 50 μ M for colorimetric assays and 5 μ M for fluorimetric assays. The Reaction Vol is 100 μ L and the Sample Vol is 10 μ L. *Notes:* if Sample OD or fluorescence values are higher than that of the Resorufin, dilute sample in Assay Buffer, repeat assay and multiply results by the dilution factor, n .

Unit definition: one unit of enzyme will catalyze the formation of 1 μ mole resorufin per min under the assay conditions.


GENERAL CONSIDERATIONS

Incubation time. Both luciferase reactions are fast, so it is recommended that samples are read as soon as possible after addition of each reagent, preferably within 1 min.

Cell number. For assay optimization, it is recommended that the optimal number of cells per well be determined by serial dilution of cells.

DATA ANALYSIS

The light intensity (RLU) is directly proportional to the luciferase concentration. For each individual sample, the RLU of the experimental reporter should be normalized by RLU of the control reporter.

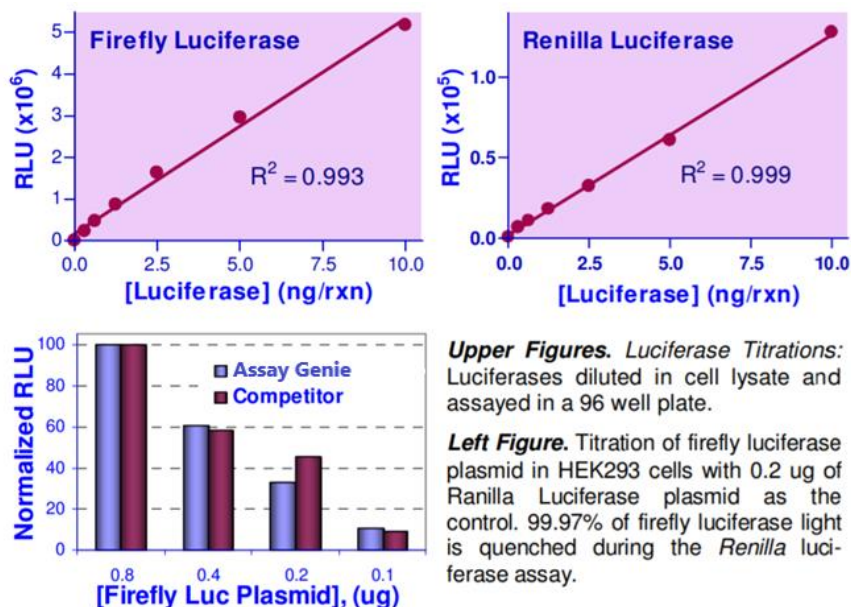

Contact Details

Dublin, Ireland

Email: info@assaygenie.com

Web: www.assaygenie.com

Technical Support: Techsupport@assaygenie.com

Copyright © 2017 ReagentBio, All Rights Reserved. All information / detail is correct at time of going to print.