

Data sheet

ROS Detection Assay kit (DCFDA / H₂DCFDA)

Cat No: CV0022 (5 x 96 assays)

Introduction:

Reactive oxygen species (ROS) include a number of reactive molecules and free radicals, derived from molecular oxygen, that damage DNA and RNA and oxidize proteins and lipids (lipid peroxidation). The most common ROS include superoxide anion (O₂^{•-}), hydrogen peroxide (H₂O₂), hydroxyl radical (HO[•]) and singlet oxygen (¹O₂), all of which are more reactive than oxygen (O₂) itself.

The molecules are produced during the electron transport of mitochondrial aerobic respiration or by oxidoreductase enzymes and metal catalysed oxidation.


Kit Contents:

| | Amount |
|--|--------|
| Fluorescent Substrate (H ₂ DCFDA) | 5 mg |
| 10X Assay Buffer | 50 ml |
| Positive Control: H ₂ O ₂ (8.8M) | 500 µl |
| DMSO | 1 ml |

Storage: 2-8°C

ROS Detection Assay kit uses the cell permeant reagent Dichlorodihydrofluorescein diacetate (H₂DCFDA), a fluorogenic dye that measures hydroxyl, peroxy and other reactive oxygen species (ROS) activity within the cell. After diffusion into the cell, the acetyl groups on H₂DCFDA are cleaved by intracellular esterase to yield the non-fluorescent compound which is rapidly oxidized to highly fluorescent 2',7'-

Dichlorodihydrofluorescein by ROS (See figure). The fluorescence intensity is proportional to the ROS levels within the cell cytosol.

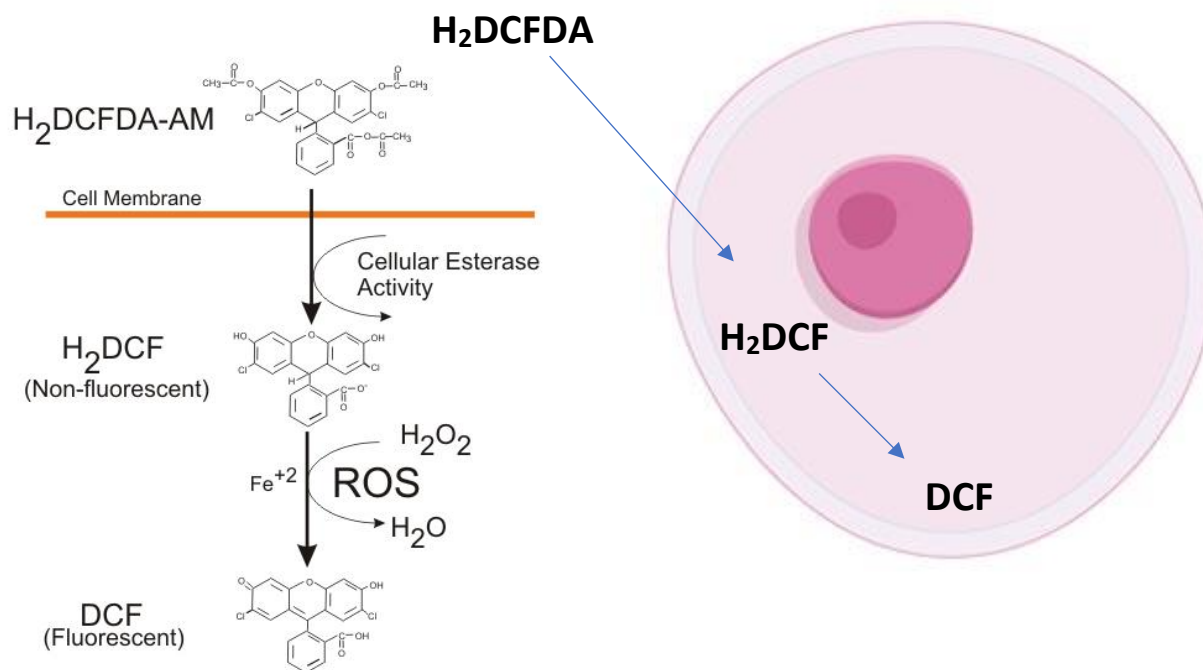

Preparation of DCF-DA stock solution:

H₂DCFDA is supplied lyophilized and should be reconstituted in 500µl DMSO to yield a 20mM stock solution. Upon reconstitution, the stock solution should be stored at -20°C to -80°C in the dark. Gently mix before use. Avoid multiple freeze/thaw cycles.

Hydrogen Peroxide (H₂O₂): Prepare H₂O₂ dilutions in 1X Assay Buffer. Do not store diluted solutions. Hydrogen Peroxide may be used as a positive control in the assay, or as a cell treatment.

Assay procedure

- Equilibrate all materials and prepared reagents to room temperature prior to use.
- It is recommended to assay all controls and samples in duplicate or triplicate.
- It is recommended to use black plates for fluorometric assays.

A - Preparation of working solutions

1. Prepare **1X Assay Buffer** by adding 10 mL 10X Assay Buffer to 90 mL deionized water. Mix gently and thoroughly.
2. Prepare a **working H₂DCFDA** solution by adding the appropriate volume of 20 mM H₂DCFDA to 1X Assay Buffer.


Vortex to evenly disperse the dye. Vortexing for about 15 to 30 seconds is usually optimal. Excessive vortexing may hasten decomposition of the dye, as it is subject to hydrolysis; on the other hand, shorter vortexing times may result in incomplete dispersion of the dye.

The exact concentration of DCFDA required will depend on the cell line being used but a general starting range would be 10 - 50 μ M. Exact concentrations have to be determined on an individual basis by the end user. This solution is unstable and must be used immediately for staining cells in culture.

B - Assay



ADHERENT CELLS

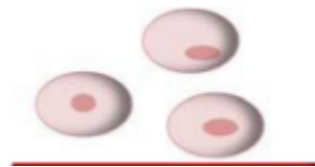

SUSPENSION CELLS

1. Stain cells in 1X buffer containing the probe (working H₂DCFDA solution) to provide a final working concentration of ~1–50 μ M dye (100 μ L per well for a 96-well format). The optimal working concentration for your application must be empirically determined.
2. Incubate at 37°C for 30–60 minutes.
3. Wash cells once in 1X Assay Buffer. Add 100ul/well of treatment
4. Treat the cells with the test ROS inducing agents or H₂O₂ (Positive control: concentrations between 25 - 100 μ M).
5. Incubate for desired period of time. Proper incubation time may need to be determined experimentally.
6. The intensity of the signal can be easily measured using a fluorescence microplate reader at Ex/Em = 485/530 nm, or a fluorescent microscope with TRITC filter or a flow-cytometry in FL1 channel.



Contact Us:

Reagent Genie Ireland Limited
G1, The Steelworks
Dublin
Ireland
D01 KA00

Email: info@reagentgenie.com

Phone: 00-353-1-887-9802