Recombinant IGFBP7 Monoclonal Antibody

Description

This Recombinant IGFBP7 Monoclonal Antibody is supplied as a kit for advanced applications. The kit includes Bradford Reagent to quantify total protein concentration for accurate sample normalization (Optional).

Product Information

SKU:	RMEA0065
Contents:	Recombinant IGFBP7 Monoclonal Antibody (50 µL, 100 µL) Bradford Reagent: 1 vial (2ml)
Clone:	C310051
Applications:	WB, IHC-P, ICC/IF, FC
Reactivity:	Human


Antibody Data

Uniprot ID:	Q16270
Size:	50 µL, 100 µL
Host Species:	Rabbit
Isotype:	Rabbit IgG
Conjugation:	Unconjugated
Buffer:	0.2 µm filtered solution in PBS


Preparation & Storage

Storage:	Store at -20°C Valid for 12 months. Avoid freeze / thaw cycles. Store Bradford Reagent at Room Temperature for 1 Year.
Shipping:	Gel Pack
Preparation:	WB: 1:1000-1:5000 ; IHC-P: 1:100-1:200 ; ICC/IF: 1:100 ; FC: 1:50-1:100
Protein Quantification (Optional):	To quantify total protein levels, use the Bradford Reagent included in this kit. Visit https://www.assaygenie.com/bradford-protein-assay-protocol/ to view the full protocol
Notes:	Centrifuge before opening to ensure complete recovery of vial contents.


Validation Data

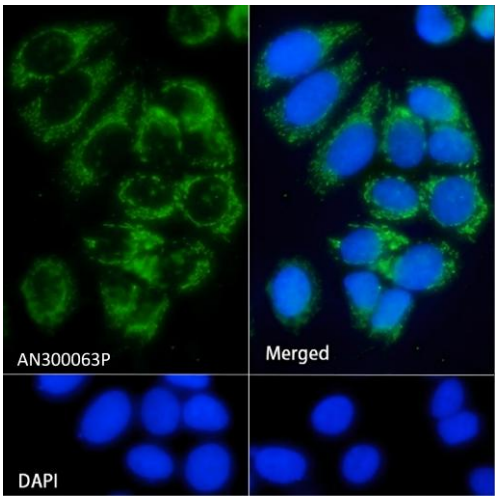


Immunofluorescence analysis of MCF-7 cells labelling IGFBP7. Nuclear DNA was labeled in blue with DAPI. Control: Secondary antibody only.

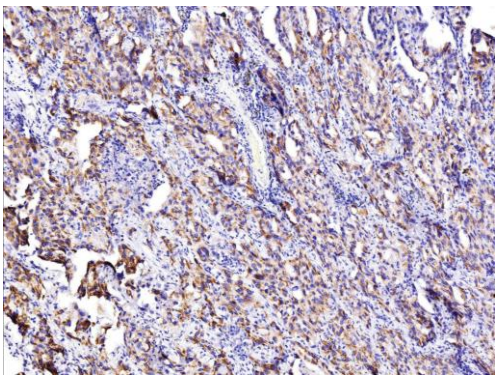

Immunohistochemical analysis of paraffin-embedded Human lung tissue sections using IGFBP7 Antibody (RMEA0065) at a dilution of 1:150 (10× lens). Heat mediated antigen retrieval was performed with Tris-EDTA buffer (pH 9.0) for 20 min prior to IHC staining.

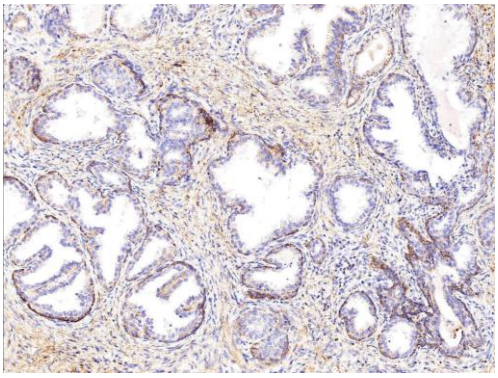

Immunohistochemical analysis of paraffin-embedded Human prostate tissue sections using IGFBP7 Antibody (RMEA0065) at a dilution of 1:150 (10× lens). Heat mediated antigen retrieval was performed with Tris-EDTA buffer (pH 9.0) for 20 min prior to IHC staining.

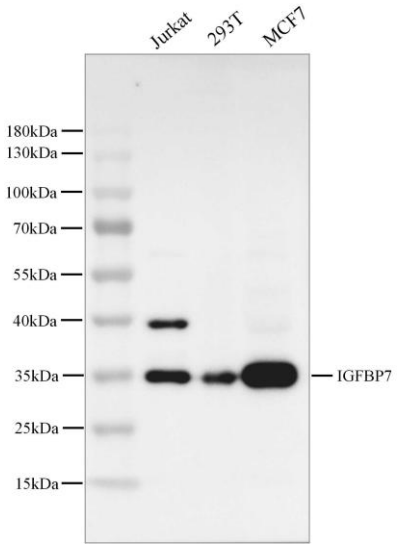

Western blot analysis of Jurkat,293T and MCF7 cell lysates using IGFBP7 Antibody (RMEA0065) at a dilution of 1:1500. Observed-MW:29 kDa Calculated-MW:29 kDa

Manufacturers Statement

This final kit system is assembled and quality-released by Assay Genie Limited.