# Recombinant METTL3 Monoclonal Antibody

## Description

This Recombinant METTL3 Monoclonal Antibody is supplied as a kit for advanced applications. The kit includes Bradford Reagent to quantify total protein concentration for accurate sample normalization (Optional).

## Product Information

| | |
|---|---|
| **SKU:** | RMEA0692 |
| **Contents:** | Recombinant METTL3 Monoclonal Antibody (50 µL, 100 µL)<br>Bradford Reagent: 1 vial (2ml) |
| **Clone:** | C110688 |
| **Applications:** | WB, IHC, IF, IP, ELISA |
| **Reactivity:** | Human, Mouse, Rat |


## Antibody Data

| | |
|---|---|
| **Uniprot ID:** | Q86U44 |
| **Size:** | 50 µL, 100 µL |
| **Host Species:** | Rabbit |
| **Isotype:** | Rabbit IgG |
| **Conjugation:** | Unconjugated |
| **Buffer:** | PBS, 50% glycerol, 0.05% Proclin 300, 0.05% protein protectant. |


## Preparation & Storage

| | |
|---|---|
| **Storage:** | Store at -20°C Valid for 12 months. Avoid freeze / thaw cycles. Store Bradford Reagent at Room Temperature for 1 Year. |
| **Shipping:** | Gel Pack |
| **Preparation:** | IHC 1:200-400, WB 1:1000-5000, IF 1:200-1000, ELISA 1:5000-20000, IP 1:50-200 |
| **Protein Quantification (Optional):** | To quantify total protein levels, use the Bradford Reagent included in this kit. Visit https://www.assaygenie.com/bradford-protein-assay-protocol/ to view the full protocol |
| **Notes:** | Centrifuge before opening to ensure complete recovery of vial contents. |


## Validation Data

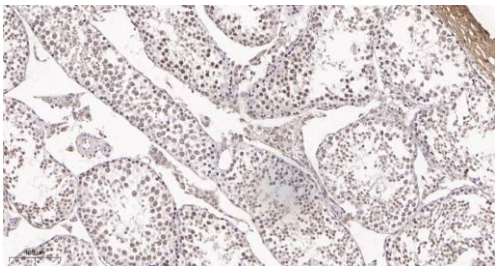


Immunohistochemistry of paraffin-embedded mouse testis tissue using Recombinant METTL3 Monoclonal Antibody at dilution of 1:200.

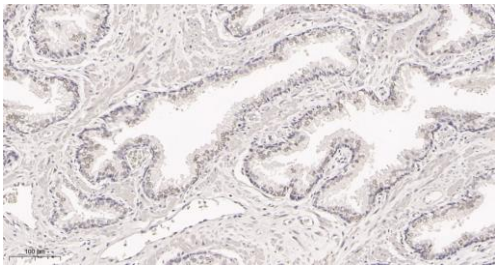

Immunohistochemistry of paraffin-embedded prostate cancer tissue using Recombinant METTL3 Monoclonal Antibody at dilution of 1:200.

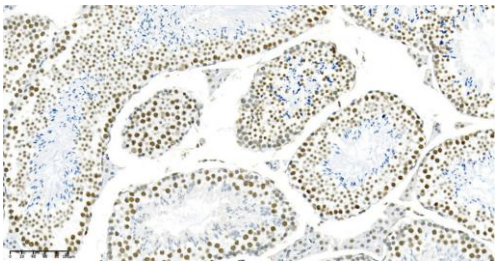

Immunohistochemistry of paraffin-embedded mouse testicles using Recombinant METTL3 Monoclonal Antibody at dilution of 1:200.

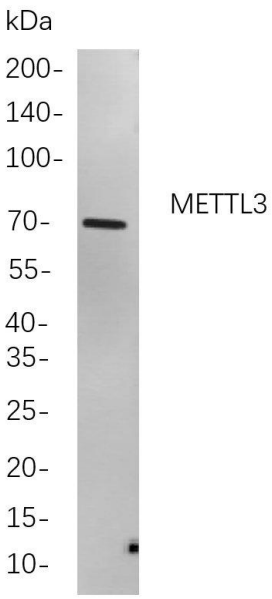


Western Blot with Recombinant METTL3 Monoclonal Antibody at dilution of 1:1000 dilution. Lane A: NCCIT cells. Observed-MW:70 kDa Calculated-MW:64 kDa

**Manufacturers Statement**

This final kit system is assembled and quality-released by Assay Genie Limited.